

Easy

Stable fecal extraction

- Maximum workflow optimisation
- Setting the standard for easy fecal extraction
- Stable at room temperature



The prefilled tubes are ready to use in three simple steps:


1

Dip the dosing tip into the fecal sample and fill the grooves completely with the matrix. 2


Place the pin back into the tube, close tightly and extract by soaking and vortexing. 3

For turbidimetric assays only: Centrifuge the extract within the CALEX® tube for 10 min.

The resulting extract (1:500) is ready to use in the turbidimetric assay. The CALEX® extraction is highly correlating to the manual weighting method.

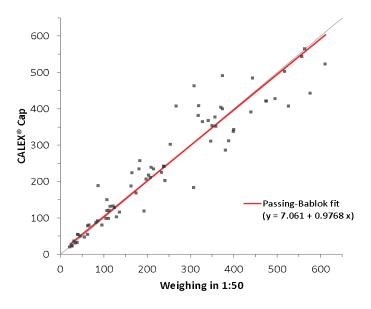

Comparison of CALEX® Cap and manual extraction. $r^2 = 0.9$

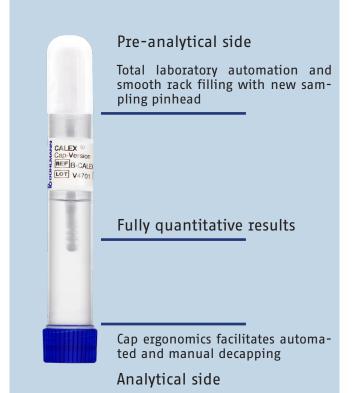

SIMPLICITY Cap ergonometry supports the simple and safe use of CALEX® Cap, significantly

reducing hands-on time

AUTOMATION Designed for total laboratory automation (TLA) systems

STABILITY Extensive validation proves stability at RT for 7 days. The CALEX® Cap is suitable

for air transportation according to IATA 650 (UN3373)


EFFICIENCY Optimal extract dilution of 1:500



From the Patient ...



...in turbo speed...



...to the Lab



BÜHLMANN Laboratories AG Baselstrasse 55 4124 Schönenbuch Switzerland



50 Valleywood Drive Markham, Ontario L3R 6E9 800.387.9643 800.268.1150 Français 905.470.2381 Fax inter-medico.com



Ordering Codes: B-CALEX-C50 B-CALEX-C200 B-CALEX-C500

50 devices 200 devices 500 devices

C€-marked products

CALEX® is a registered trademark of BÜHLMANN in many countries.

Parts of the CALEX® Cap are patent protected by:
EP2833795(B1); US9752967(B2); AU2016203121(B2); CA2997598(C);
JP6307132(B2); KR10-1875862(B1).